





CAM Operation w/ Model HPP125/ HP125 Probes		
CAM OPERATION NOTE	Reference Only	
	RJN	March 16-16
Edgetech Instruments Inc.	SK-O-HP-03162016A	

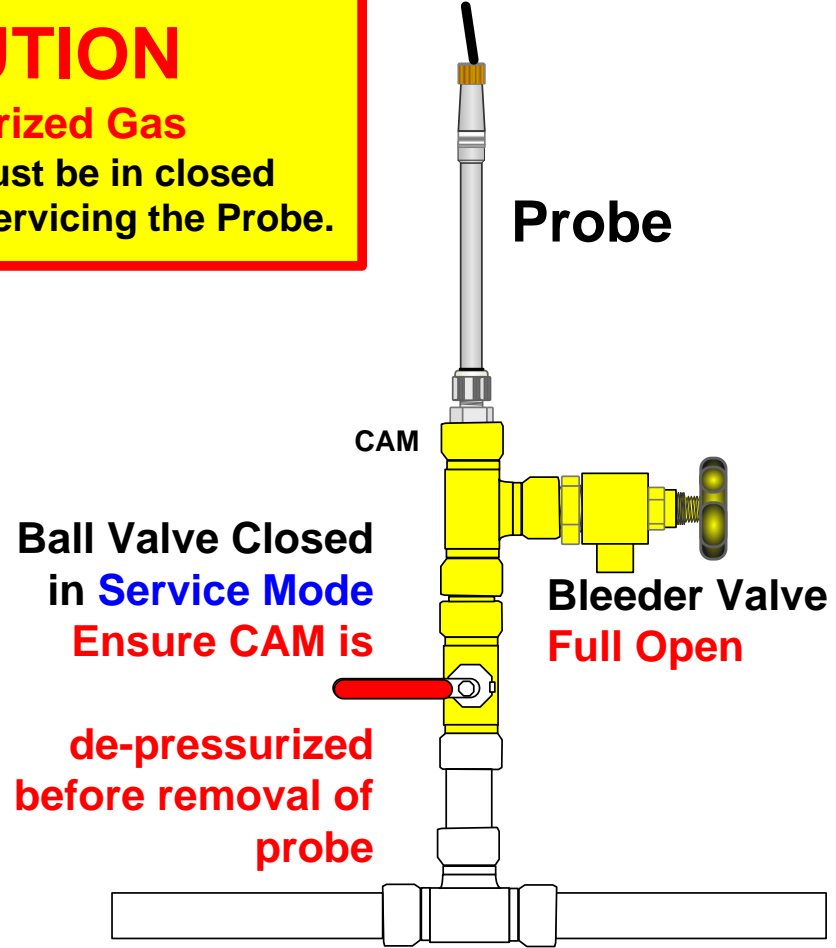


CAUTION
Pressurized Gas
Ball Valve must be in closed position when servicing the Probe.

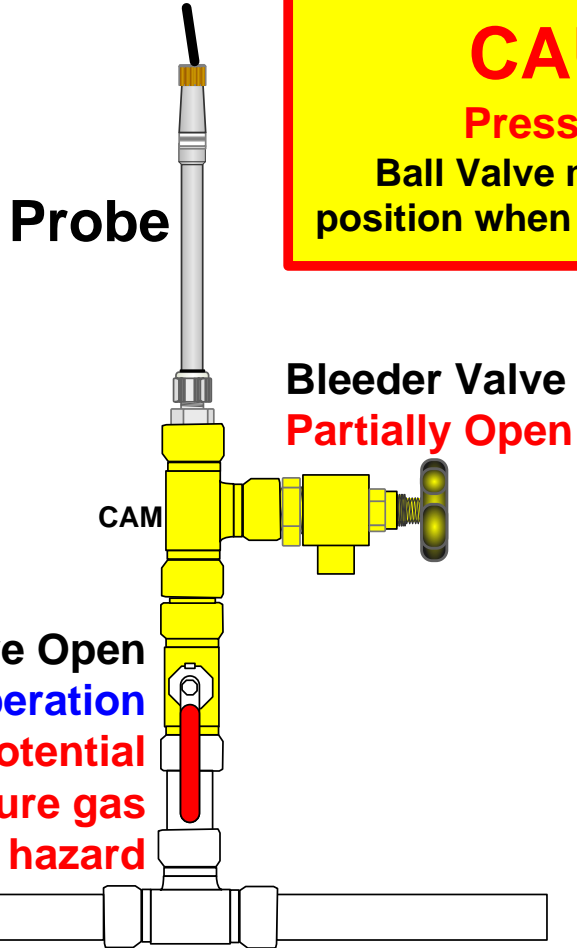


HAZARD WARNING CAM OPERATION		
CAM OPERATION	Reference Only	
	RJN	MARCH 16, 16
Edgetech Instruments Inc.	SK-WL-03162016A	

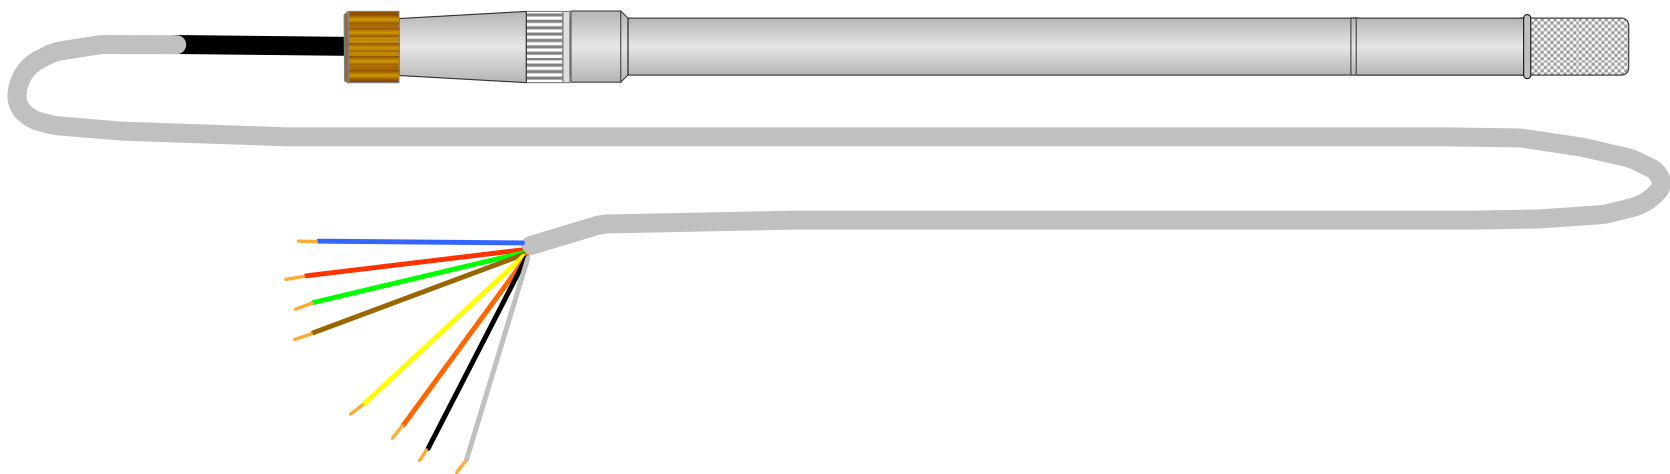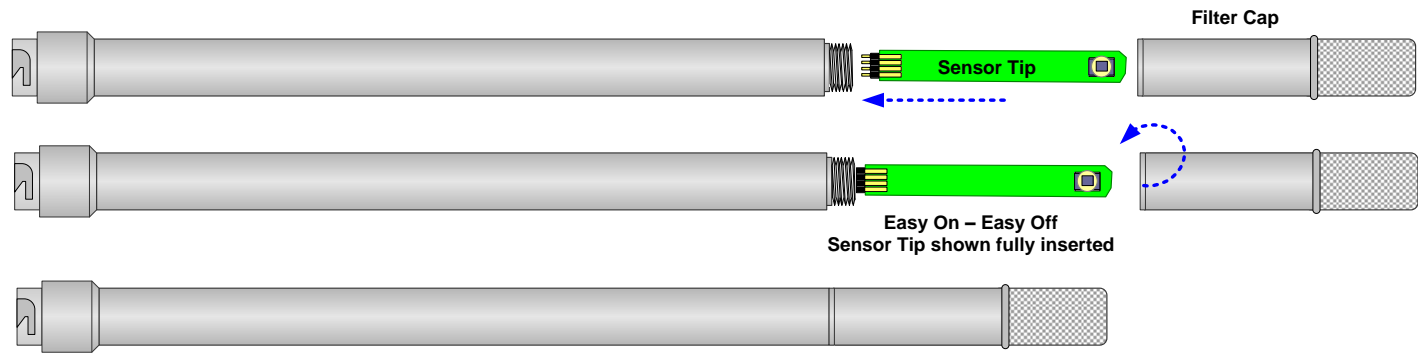


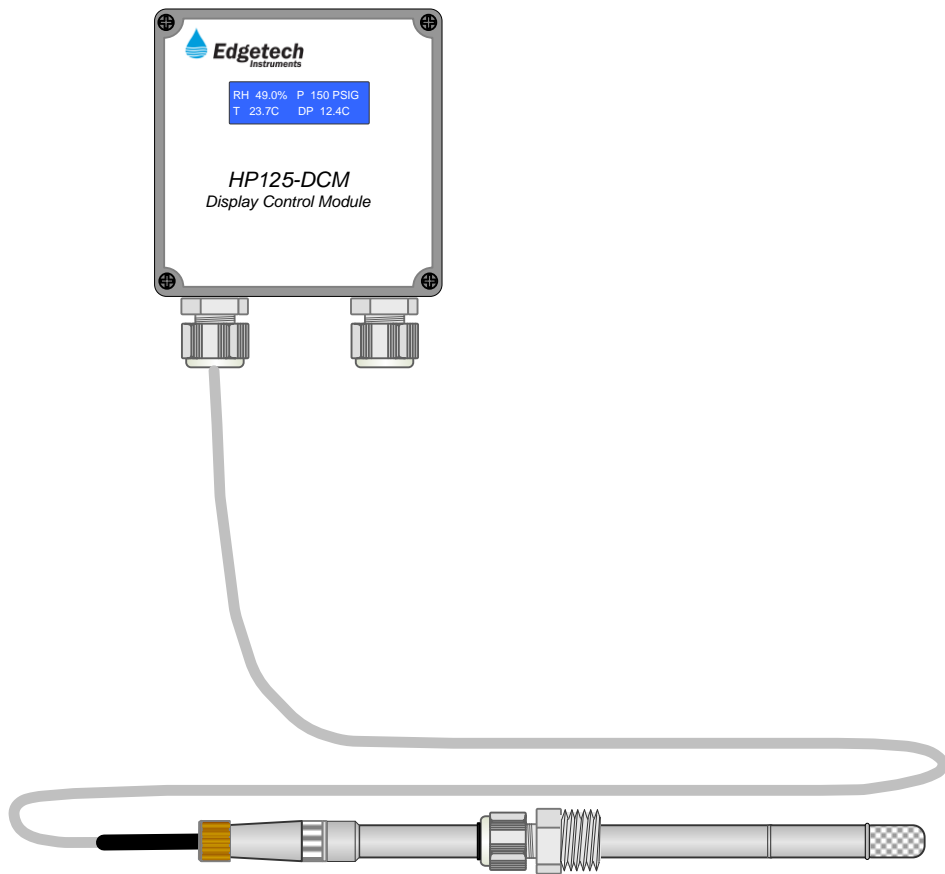


STANDARD MALE CONNECTOR MOUNT
1/2 in NPT or 3/4in NPT

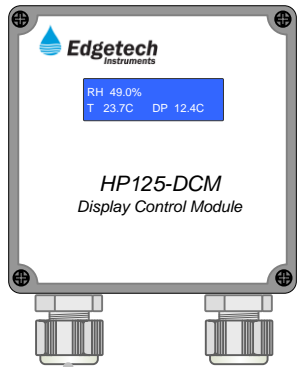


OUTPUTS
Analog Voltage & 4-20 mA
RS-232 Serial Interface
Alarm Relays
Standard 24 VDC Power

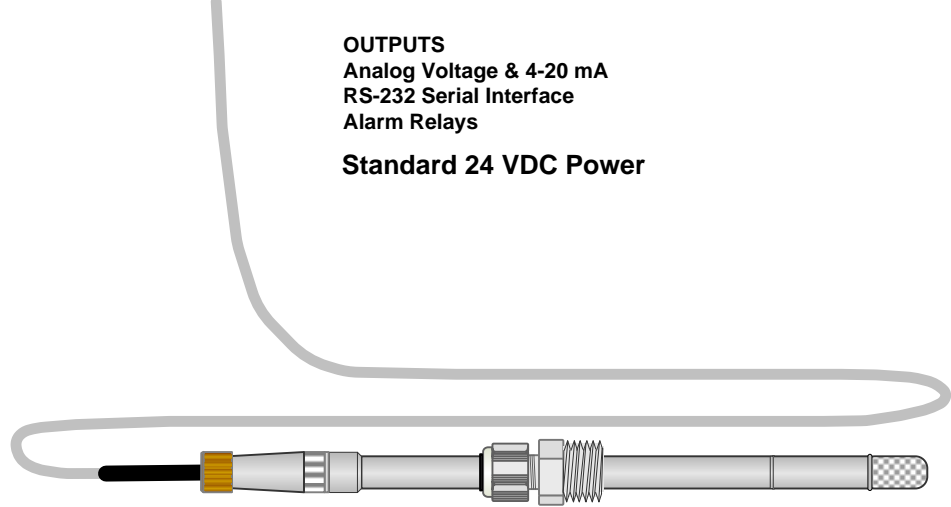


STANDARD MALE CONNECTOR MOUNT
 $\frac{1}{2}$ in NPT or $\frac{3}{4}$ in NPT

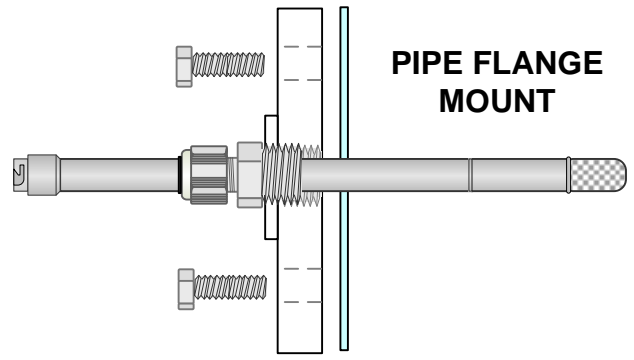

PIPE FLANGE MOUNT

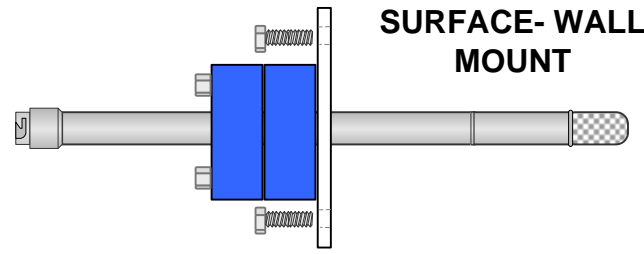

SURFACE-WALL MOUNT

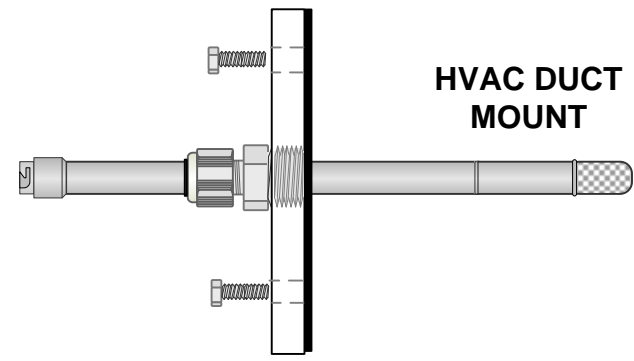

HVAC DUCT MOUNT

Probe Penetration Fitting

Adjustable Depth into process penetration point

Standard: 1/2" or 3/4" NPT

Metric Thread Sizes available

